



Evaluation of body fluid mode of Sysmex XN-9000 for white blood cell counts in cerebrospinal fluid

Vincenzo Roccaforte¹, Massimo Daves², Vanessa Proserpio¹, Flavia Sciarini¹, Rosella Sangiorgio¹, Arcangelo Costanzo¹, Angela M. Di Pierro³, Salvadori Ugo², Giuseppe Lippi⁴, Claudio Bonato¹

¹Clinical Pathology Laboratory, Hospital of Lecco, Lecco, Italy; ²Transfusion Center, Hospital of Bolzano, Bolzano, Italy; ³Clinical Pathology Laboratory, Hospital of Bolzano, Bolzano, Italy; ⁴Section of Clinical Biochemistry, University of Verona, Verona, Italy

Contributions: (I) Conception and design: V Roccaforte; (II) Administrative support: None; (III) Provision of study materials or patients: F Sciarini, V Proserpio; (IV) Collection and assembly of data: V Roccaforte, M Daves; (V) Data analysis and interpretation: V Roccaforte, G Lippi; (VI) Manuscript writing: All authors; (VII) Final approval of manuscript: All authors.

Correspondence to: Vincenzo Roccaforte. Clinical Pathology Laboratory, Hospital Alessandro Manzoni, Street Eremo 9/11, 23900 Lecco, Italy.
Email: v.roccaforte@asst-lecco.it.

Background: This study was planned to evaluate the analytical performance of the novel and fully automated Sysmex XN-9000 analyzer for rapid analysis of cerebrospinal fluid (CSF) samples.

Methods: Forty-four CSF samples were used for method comparison studies between Sysmex XN-9000 body fluid mode and conventional optical microscopy. The bias between data obtained with the two methods was estimated with Bland-Altman plot analysis. The analytical evaluation also included the assessment of imprecision, linearity and carry-over.

Results: A good agreement was found between results obtained with Sysmex XN-9000 body fluid mode and optical microscopy. The mean bias was 1.6×10^6 cells/L for total white blood cells (95% CI: -21.8×10^6 to 25.1×10^6 cells/L), 1.3×10^6 cells/L for polymorphonuclear cells (95% CI: -13.9×10^6 to 16.5×10^6 cells/L) and -0.6×10^6 cells/L for mononuclear cells (95% CI: -21.5×10^6 to 20.3×10^6 cells/L). The carryover was found to be lower than 0.01% and the imprecision was lower than 5%. The XN-9000 body fluid mode was also characterized by excellent linearity in the range of values comprised between 85×10^6 – $3,197 \times 10^6$ cells/L, with correlation coefficients (r) always equal to 1.00 ($P < 0.001$).

Conclusions: The Sysmex XN-9000 body fluid mode displays excellent analytical performance in terms of imprecision, linearity, carry-over and comparability with conventional optical microscopy, so that it may be used as a first-line, screening technique for rapid analysis of CSF samples referred for both routine and, especially, for urgent testing.

Keywords: Cerebrospinal fluid (CSF); Sysmex XN-9000; optical microscopy; leukocytes

Received: 20 December 2017; Accepted: 31 January 2018; Published: 07 March 2018.

doi: 10.21037/jlpm.2018.02.01

View this article at: <http://dx.doi.org/10.21037/jlpm.2018.02.01>

Introduction

The infections of the central nervous system (CNS) are conventionally classified as meningitis or encephalitis. The analysis of white blood cells (WBC) in cerebrospinal fluid (CSF) is a key diagnostic element for the different diagnosis of a kaleidoscope of diseases, thus including inflammatory conditions and infectious or non-infectious disorders

involving the CNS (1-3).

The CSF normally contains a very low number of WBC. In adults, the number of nucleated cells in the CSF is conventionally $< 5.0 \times 10^6$ cells/L, whilst their count should remain below 7.0×10^6 cells/L in the CSF of children and below 30.0×10^6 cells/L in that of neonates, respectively (4). The presence of a high number of WBC may hence be suggestive, or even diagnostic, for an

infection, for diseases such as meningitis and encephalitis, or for other neurological disorders (1,5). The normal cellular components of CSF include mainly lymphocytes (i.e., approximately 70%, mostly T-cells) and monocytes (i.e., approximately 30%). Neutrophils are not normally present in CSF, and their occasional observation in non-pathological CSF samples can be attributed to a microscopic contamination during lumbar puncture, which is then magnified by cytocentrifugation. Therefore, occasional finding of rare neutrophils in CSF is not necessarily a hallmark of a pathological condition (4).

Optical microscopy is still regarded as the “gold standard” for identification and enumeration of WBC in CSF (4,6). Nevertheless, this technique has some well-known drawbacks, such as the relatively high inaccuracy, low imprecision, lengthy turnaround time (TAT) and the need to educate and train specialized personnel for this type of manual analysis (7). A new generation of fully-automatic hematologic analyzers has been developed and commercialized in recent years. In 2006, the Sysmex (Kobe, Japan) *in vitro* diagnostic (IVD) company has integrated a specific body fluid (BF) mode on its XE-5000 analyzer, which is hence mainly aimed to be used for analysis of biological fluids other than blood, so mainly including CSF, ascites, synovial, pericardial and pleural fluids. This mode not only exhibits acceptable analytical performance, but also displays many potential advantages for laboratory workout and organization, mostly attributable to the faster TAT and the more cost-effective management of specimens than using optical microscopy (8-10). Nevertheless, high imprecision in CSF samples with a number of WBC $\leq 20 \times 10^6/L$, probably due to overestimation of polymorphonuclear cell (PMN) counts, was an important shortcoming that has been highlighted in some previous investigations (11-13).

Therefore, the aim of study was to assess the analytical performance of the novel and fully automated Sysmex XN-9000 BF mode for identification and enumeration of WBC in CSF, as well as the evaluation of its basic analytical performance.

Methods

Analyzer description

The new automated haematology analyser Sysmex XN-9000 (Sysmex, Kobe, Japan) can operate either in “whole blood” mode, or with a second mode dedicated to BF

analysis (i.e., BF mode). The analytical performance of the whole blood mode has been recently and exhaustively evaluated (14,15). The second mode, specifically dedicated to BF analysis, entails the use of an innovative software, which allows enumeration and classification of WBC, PMN, mononuclear (MN) and high fluorescent BF (HF-BF) cells in the “DIFF” channel according to their side scatter (so reflecting internal complexity) and fluorescence intensity (i.e., mirroring DNA/RNA content) (4,16,17). The analyzer only uses 88 μL for each BF sample analysis. A rinsing cycle is also activated before starting a new test, thus preventing spurious contamination from material of the previous sample.

Study design

The comparison study was carried out using 44 CSF samples referred to the local laboratory for routine analysis. All samples were tested within 1 h from arrival in the laboratory. CSF collection and analysis of cellular composition were performed in accordance with the Clinical and Laboratory Standards Institute (CLSI) document H56-A (4). The results of total WBC count were directly compared with those obtained on the same CSF sample by optical microscopy on Nageotte chamber, after staining with Turk’s solution. The slides for differential WBC count were prepared with cytopsin (Shandon Cytospin 3 centrifuge; Thermo Shandon, Cergy Pontoise, France), starting from 200 μL of CSF. The slides were then stained with May-Grunwald-Giemsa, using a Sysmex SP-10 slide-stainer unit (Sysmex, Etten-Leur, The Netherlands). Microscopic analysis was performed with light microscopy under oil immersion, at 50 \times magnification. Two independent experts performed all the microscopic analyses, and the individual results were then averaged to obtain the final count. The bias [and its 95% confidence interval (CI)] between data obtained with either optical microscopy or Sysmex XN-9000 BF mode was estimated with Bland-Altman plot analysis.

The within-run precision of the BF mode on XN-9000 was evaluated with 20 consecutive measurements of two CSF samples with low (mean value, 36×10^6 cells/L) and high (mean value, $1,346 \times 10^6$ cells/L) WBC counts. The imprecision was finally expressed in percentage, as coefficient of variation (CV), according to the CLSI document EP5-A2 (18).

Carry-over was assessed by measuring a CSF sample with high cell count in triplicate (H1, H2, H3), followed by

Table 1 Main results of comparison study using 44 cerebrospinal fluid (CSF) analyzed with Sysmex XN-9000 body fluid mode and optical microscopy (results are shown as $\times 10^6$ cells/L)

CSF parameter	Body fluid	Optical microscopy
WBC	Lowest value: 0	Lowest value: 0
	Highest value: 662	Highest value: 680
	Mean: 48.9	Mean: 47.3
	Standard deviation: 117.35	Standard deviation: 121.73
	Standard error of the mean: 17.69	Standard error of the mean: 18.35
MN	Lowest value: 0	Lowest value: 0
	Highest value: 317	Highest value: 360
	Mean: 25.4	Mean: 24.9
	Standard deviation: 63.3	Standard deviation: 59.9
	Standard error of the mean: 9.03	Standard error of the mean: 9.54
PMN	Lowest value: 0	Lowest value: 0
	Highest value: 619	Highest value: 640
	Mean: 23.8	Mean: 22.5
	Standard deviation: 94.77	Standard deviation: 97.05
	Standard error of the mean: 14.29	Standard error of the mean: 14.63

WBC, white blood cells; MN, mononuclear cells; PMN; polymorphonuclear cells.

three consecutive measurements of blank solution (Cellpack; L1, L2, L3). The final result was calculated as follows: $[(L1-L3)/(H3-L3)] \times 100$, as currently recommended by the International Council for Standardization in Haematology (ICSH) (19).

The linearity was assessed measuring two CSF samples with different cell counts (sample A: WBC, $3,197 \times 10^6$ cells/L; sample B: WBC, 85×10^6 cells/L). Each sample was serially diluted with Cellpack to obtain scalar values, which were then measured three consecutive times each. Results were then compared with expected values, as for indications of CLSI document EP06-A (20).

Statistical analysis

The statistical analysis was performed using MedCalc statistical package (version 17.6, MedCalc Software, Mariakerke, Belgium).

Results

The main results of this study are shown in *Table 1*. The overall bias between the Sysmex XN-9000 BF mode and

optical microscopy was always clinically meaningless. In particular, the Bland-Altman plot analysis allowed to estimate a mean bias with optical microscopy of 1.6×10^6 cells/L (95% CI: -21.8×10^6 to 25.1×10^6 cells/L) for total WBC, 1.3×10^6 cells/L (95% CI: -13.9×10^6 to 16.5×10^6 cells/L) for PMN, and -0.6×10^6 cells/L (95% CI: -21.5×10^6 to 20.3×10^6 cells/L) for MN, respectively (*Figure 1*).

The XN-9000 body fluid mode also displayed excellent linearity throughout a broad range of clinically significant values (i.e., between 85×10^6 – $3,197 \times 10^6$ cells/L), with all correlation coefficients for WBC, PMN and MN equal to 1.00 ($P < 0.001$). The carryover was negligible (i.e., $< 0.01\%$), and the imprecision excellent, with CVs $< 5\%$ and $< 4\%$ for CSF samples with mean values of 36×10^6 WBC/L and $1,346 \times 10^6$ WBC/L, respectively.

Discussion

The accurate identification and enumeration of cells in CSF are essential needs for rapid diagnosis and appropriate therapeutic treatment of patients with CSF disorders. Optical microscopy, using the so-called “counting chambers” (i.e., Fuchs Rosenthal, Burker, Neubauer or

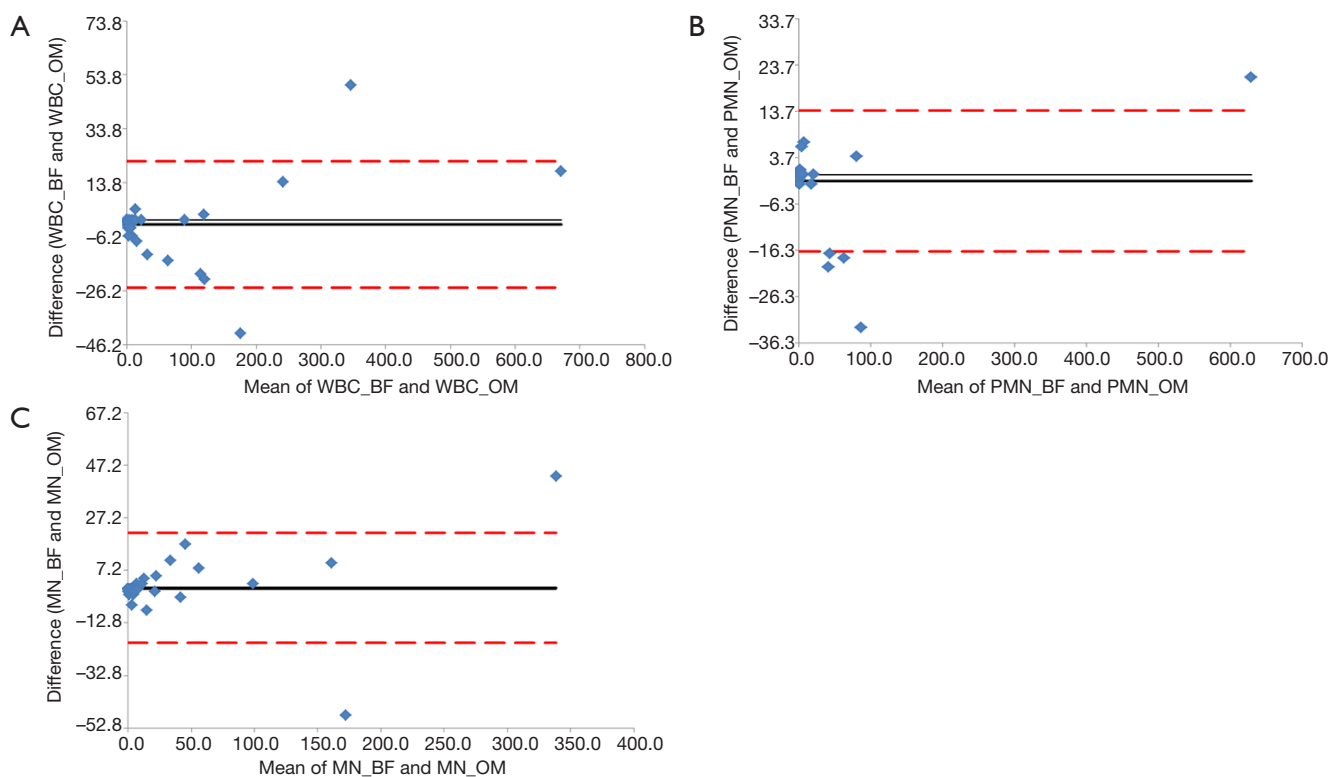


Figure 1 Bland and Altman plot analysis for total white blood cells (WBC) (A), polymorphonuclear cells (PMN) (B) and mononuclear cells (MN) (C) in 44 cerebrospinal fluid (CSF) samples analyzed with Sysmex XN-9000 body fluid mode (BF) and optical microscopy (OM) (results are shown as $\times 10^6$ cells/L).

Nageotte), remains “gold standard” for total WBC and erythrocyte counts in this BF, whilst stained cytocentrifuged slides are typically used for differentiating WBC into MN and PMN (8,13).

The considerable technological advancements occurred in recent years have allowed to introduce a new generation of automated hematological analyzers in routine clinical laboratories, which are now increasingly used for cell identification and counting in samples other than whole blood. For certain types of BF, automated cell count has hence allowed to achieve a high degree of accuracy and precision, concomitantly reducing both inter-observer variability and TAT (21,22), even if some doubts remain about their reliability in BF samples with low cellularity (9,10,23). In a previous evaluation of the Sysmex XE-5000 BF mode, Fleming *et al.* found a good agreement with optical microscopy for WBC ($r=0.97$) and MN ($r=0.93$) counts, whereas a less satisfactory concordance was observed for the PMN count ($r=0.87$) (5). Paris *et al.* (6) also showed a good correlation for total WBC ($r=0.96$) and

MN counts ($r=0.98$) between XE-5000 BF mode and optical microscopy using 81 CSF samples, which were obtained from oncology, pediatric and adult hematological patients. Notably, the poor correlation between XE-5000 BF mode and optical microscopy was confirmed in their study ($r=0.58$) (6), whilst it was also highlighted that automated testing was not efficient enough to identify blast cells, since the XE-5000 BF mode overlaps blast cells with MN, so that optical microscopy would remain mandatory in these cases (6).

Conclusions

Our study was mainly aimed to assess the analytical performance of the new BF mode on the Sysmex XN-9000 using CSF samples, and comparing data with those obtained with the reference technique (i.e., optical microscopy). Taken together, our results suggest that this BF mode displays excellent analytical performance in terms of imprecision, linearity and carry-over throughout

a broad range of cellularity in CSF samples. This data, combined with the excellent correlation with optical microscopy observed from the analysis of 44 routine CSF samples displaying heterogeneous cellularity, suggests that the Sysmex XN-9000 BF mode may be used as a first-line, screening technique for rapid analysis of CSF samples either referred for routine or, especially, for urgent testing.

Acknowledgements

None.

Footnote

Conflicts of Interest: The authors have no conflicts of interest to declare.

Ethical Statement: The investigation was entirely based on the use of routine samples referred to the local laboratory for CSF analysis, all samples were anonymized before testing, test results did not impact the clinical management of patients and, therefore, ethical approval or patient's permission to use the samples for this study were cleared by the local institutional review board. The study was performed in accordance with the Declaration of Helsinki and under the terms of all relevant local legislations.

References

- Buoro S, Seghezzi M, Mecca T, et al. Evaluation of Mindray BC-6800 body fluid mode for automated cerebrospinal fluid cell counting. *Clin Chem Lab Med* 2016;54:1799-810.
- Fleming C, Russcher H, Lindemans J, et al. Clinical relevance and contemporary methods for counting blood cells in body fluids suspected of inflammatory disease. *Clin Chem Lab Med* 2015;53:1689-706.
- de Almeida SM, Nogueira MB, Raboni SM, et al. Laboratorial diagnosis of lymphocytic meningitis. *Braz J Infect Dis* 2007;11:489-95.
- Clinical and Laboratory Standards Institute. Body fluid analysis for cellular composition; approved guidelines. CLSI document H56-A. Wayne, PA: Clinical and Laboratory Standards Institute, 2006.
- Fleming C, Brouwer R, Lindemans J, et al. Improved software on the Sysmex XE-5000 BF mode for counting leukocytes in cerebrospinal fluid. *Clin Chem Lab Med* 2013;51:e61-3.
- Paris A, Nhan T, Cornet E, et al. Performance evaluation of the body fluid mode on the platform Sysmex XE-5000 series automated hematology analyzer. *Int J Lab Hematol* 2010;32:539-47.
- Aune MW, Becker JL, Brugnara C, et al. Automated Flow Cytometric Analysis of Blood Cells in Cerebrospinal Fluid. *Am J Clin Path* 2004;121:690-700.
- de Jonge R, Brouwer R, de Graaf MT, et al. Evaluation of the new body fluid mode on the Sysmex XE-5000 for counting leukocytes and erythrocytes in cerebrospinal fluid and other body fluids. *Clin Chem Lab Med* 2010;48:665-75.
- Boer K, Deufel T, Reinhoefer M. Evaluation of the XE-5000 for the automated analysis of blood cells in cerebrospinal fluid. *Clin Biochem* 2009;42:684-91.
- Zimmermann M, Ruprecht K, Kainzinger F, et al. Automated vs. manual cerebrospinal fluid cell counts: a work and cost analysis comparing the Sysmex XE-5000 and the Fuchs-Rosenthal manual counting chamber. *Int J Lab Hematol* 2011;33:629-37.
- Perné A, Hainfellner JA, Womastek I, et al. Performance evaluation of the Sysmex XE-5000 hematology analyzer for white blood cell analysis in cerebrospinal fluid. *Arch Pathol Lab Med* 2012;136:194-8.
- Sandhaus LM, Ciarlini P, Kidric D, et al. Automated Cerebrospinal Fluid Cell Counts Using the Sysmex XE-5000. *Am J Clin Pathol* 2010;134:734-8.
- Dux R, Kindler-Rohrborn A, Annas M, et al. A standardized protocol for flow cytometric analysis of cells isolated from cerebrospinal fluid. *J Neurol Sci* 1994;121:74-8.
- Briggs C, Longair I, Kumar P, et al. Performance evaluation of the Sysmex haematology XN modular system. *J Clin Pathol* 2012;65:1024-30.
- Tanaka Y, Tanaka Y, Gondo K, et al. Performance evaluation of platelet counting by novel hematology analyzers. *J Clin Lab Anal* 2014;28:341-8.
- Lippi G, Cattabiani C, Benegiamo A, et al. Evaluation of white blood cell count in peritoneal fluid with five different hemocytometers. *Clin Biochem* 2013;46:173-6.
- Fleming C, Brouwer R, Lindemans J, et al. Validation of the body fluid module on the new Sysmex XN-1000 for counting blood cells in cerebrospinal fluid and other body fluids. *Clin Chem Lab Med* 2012;50:1791-8.
- Clinical and Laboratory Standards Institute (CLSI). Evaluation of Precision Performance of Quantitative Measurement Methods: Approved Guideline. 2nd edition. CLSI document EP5-A2. Wayne, PA: Clinical and

- Laboratory Standards Institute, 2004.
19. Guidelines for the evaluation of blood cell analysers including those used for differential leucocyte and reticulocyte counting and cell marker applications. International Council for Standardization in Haematology: prepared by the ICSH Expert Panel on Cytometry. Clin Lab Haematol 1994;16:157-74.
 20. Clinical and Laboratory Standards Institute (CLSI). Evaluation of the Linearity of Quantitative Measurement Procedures, A Statistical Approach. 1st edition. Approved Guideline. CLSI document EP6-A. Wayne, PA: Clinical and Laboratory Standards Institute, 2003.
 21. Nanos NE, Delanghe JR. Evaluation of Sysmex UF-1000i for use in cerebrospinal fluid analysis. Clin Chim Acta 2008;392:30-3.
 22. De Smet D, Van Moer G, Martens GA, et al. Use of the Cell-Dyn Sapphire hematology analyzer for automated counting of blood cells in body fluids. Am J Clin Pathol 2010;133:291-9.
 23. Barnes PW, Eby CS, Shimer G. An evaluation of the utility of performing body fluid counts on the coulter LH 750. Lab Hematol 2004;10:127-31.

doi: 10.21037/jlpm.2018.02.01

Cite this article as: Roccaforte V, Daves M, Proserpio V, Sciarini F, Sangiorgio R, Costanzo A, Di Pierro AM, Ugo S, Lippi G, Bonato C. Evaluation of body fluid mode of Sysmex XN-9000 for white blood cell counts in cerebrospinal fluid. J Lab Precis Med 2018;3:22.